

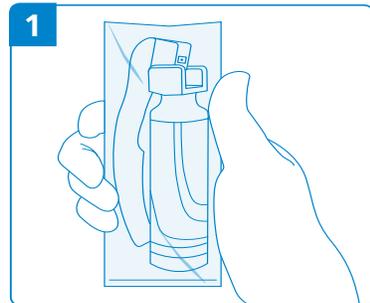


# BritePro™ Omni


BritePro Omni's **LED light** can be **tested in-pack** before opening.

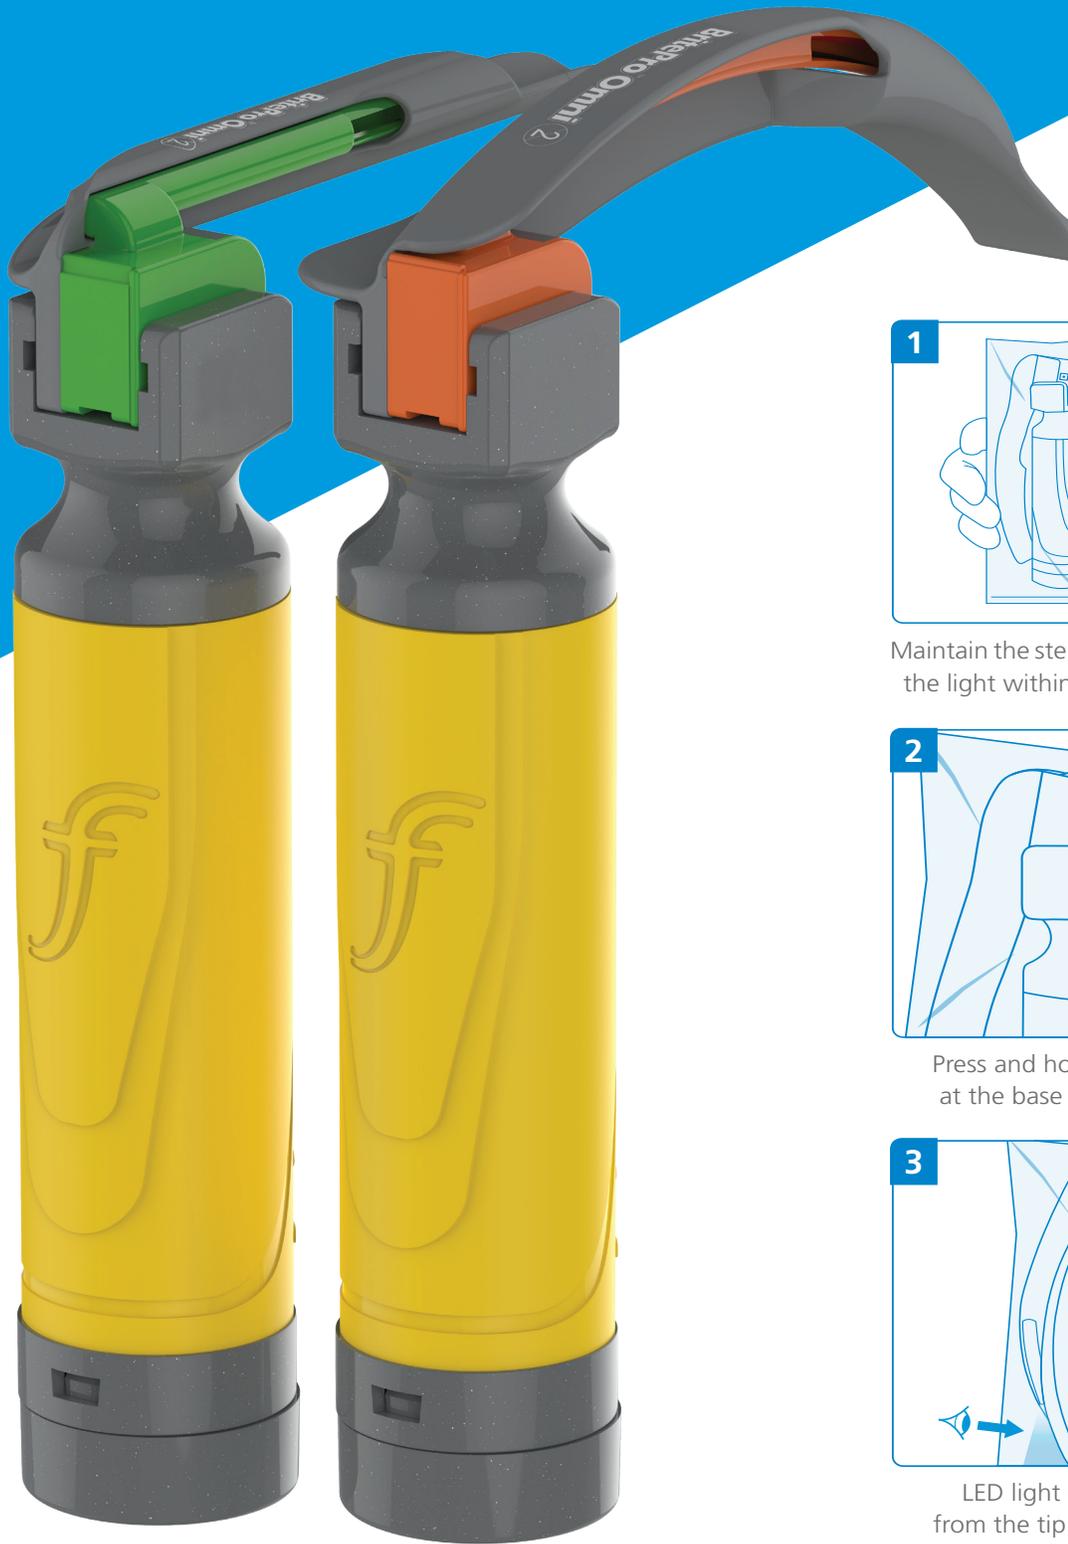

1  
Maintain the sterile seal by testing the light within the packaging.

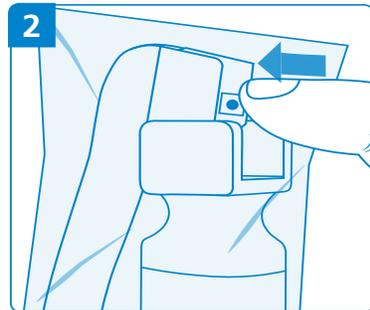

2  
Press and hold the button at the base of the blade.

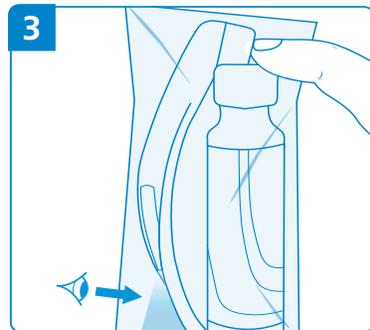

3  
LED light illuminates from the tip of the blade.