

McKESSON

Transfer Bench aluminum frame


Provides a total weight bearing capacity of 400 lbs (181 kg).

For use with MFR# 146-RTL12031KDR.

ASSEMBLY INSTRUCTIONS


1. Remove contents from carton.
2. Lay both transfer bench seat sections upside down on a flat surface.
3. Slide smaller seat section into larger section by depressing the brass push pins and inserting into the receptacles. Snap buttons will pop out when secure (Figure 1).

FIGURE 1

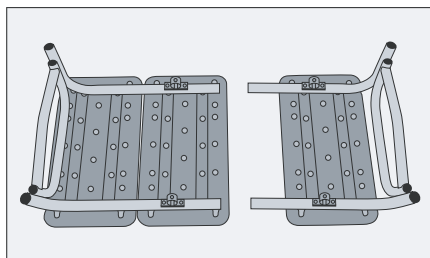


4. Remove black top from 4 leg receptacles.
5. Attach leg with the large suction cup (marked "A") by depressing the brass push pin and inserting into the receptacle with the matching "A". Repeat for second leg (Figure 2).

FIGURE 2

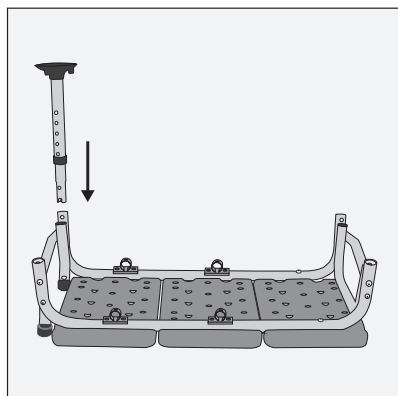


6. Attach leg with small rubber tip (marked "B") by depressing brass push pin and inserting into the receptacle with matching "B". Repeat for second leg (Figure 3).

FIGURE 3

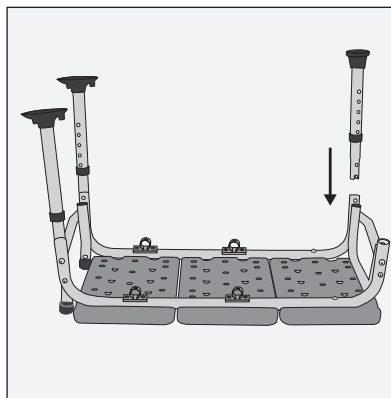


7. Turn transfer bench right-side-up. Attach armrest by depressing brass push pins and sliding into the arm receptacle on the side of the bench. Make sure the arm arcs outward, not inward (Figure 4).

FIGURE 4

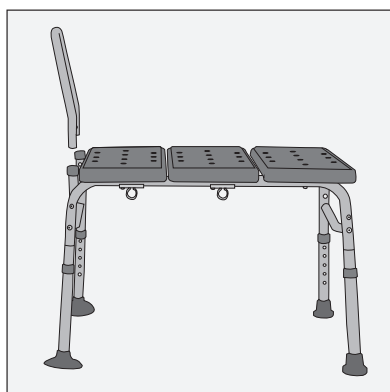

8. To assemble backrest, insert support tube into backrest support by depressing push pin and sliding into backrest tube. Repeat for second support tube (Figure 5).


FIGURE 5

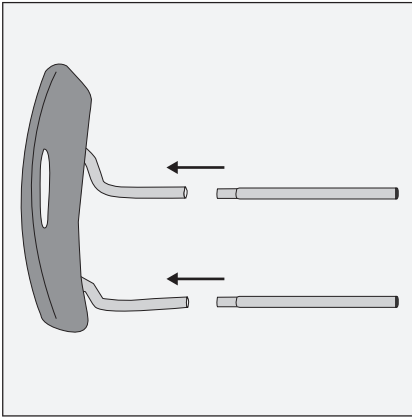

9. Insert backrest into base by depressing push pins and sliding support tubes through both receptacles.

NOTE: Backrest must go through both sets of receptacles to become secure (Figure 6).

FIGURE 6

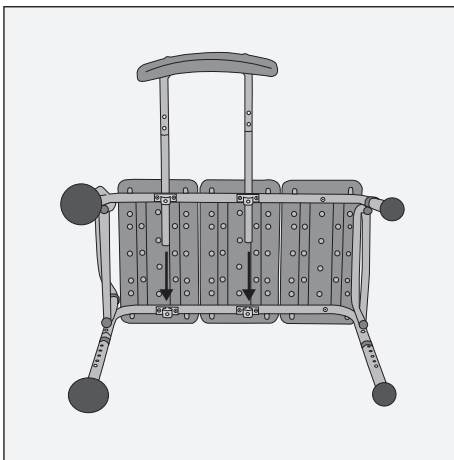

NOTE: Back support is reversible to accommodate left or right tub entry. You can also change the seat depth of your transfer bench by pushing the pins under the seat and sliding the tubes forward until the pins lock into place.

8. Place legs with the large suction cups into bath tub.

ADJUSTING LEG HEIGHT

1. To adjust leg height, remove U-Clip adjustment hole, set leg to desired height and return U-clip into adjustment hole. Make sure U-Clip clicks into place. Repeat for remaining legs.

NOTE: Make sure all legs are set to the same height.

2. To be sure legs are locked into place, push down or pull up on legs.

ADDITIONAL PRECAUTIONS

1. Inspect all parts for shipping damage before assembly. If there is shipping damage - DO NOT USE. Contact dealer/carrier for further instructions.
2. Make certain that the snap buttons fully protrude through the same respective holes of each leg extension. This will ensure that the leg extensions are securely locked in position and an even height is achieved.
3. Ensure ALL screws, nuts and/or bolts are tightened.
4. Check the rubber tips on the leg extensions for rips, wear or if they are missing. Immediately replace any or all if any of these imperfections exist.
5. All four leg extensions with rubber tips MUST touch the floor simultaneously at all times.
6. DO NOT stand on the bench.

NOTE: To maintain the beauty of the original finish, clean with mild soap and rinse with warm water. Wipe seat dry after each use.

Technical support, replacement parts and warranty information? Call 1-866-694-5085.
General product questions? Call 1-800-777-4908

Satisfaction Guaranteed

For complete details, please visit
mms.mckesson.com/mckesson-brands.

Distributed by McKesson Medical-Surgical Inc.
Richmond, VA 23233
PVN B0518
Made in China